


Effects of Sterilization and 1-Year Real-Time Aging on Material Tensile Strength (MD) for 1073B




Transition Protocol material performance is equivalent to, or better than, current Tyvek®.

Effects of Sterilization and 1-Year Real-Time Aging on Material Tensile Strength (CD) for 1073B

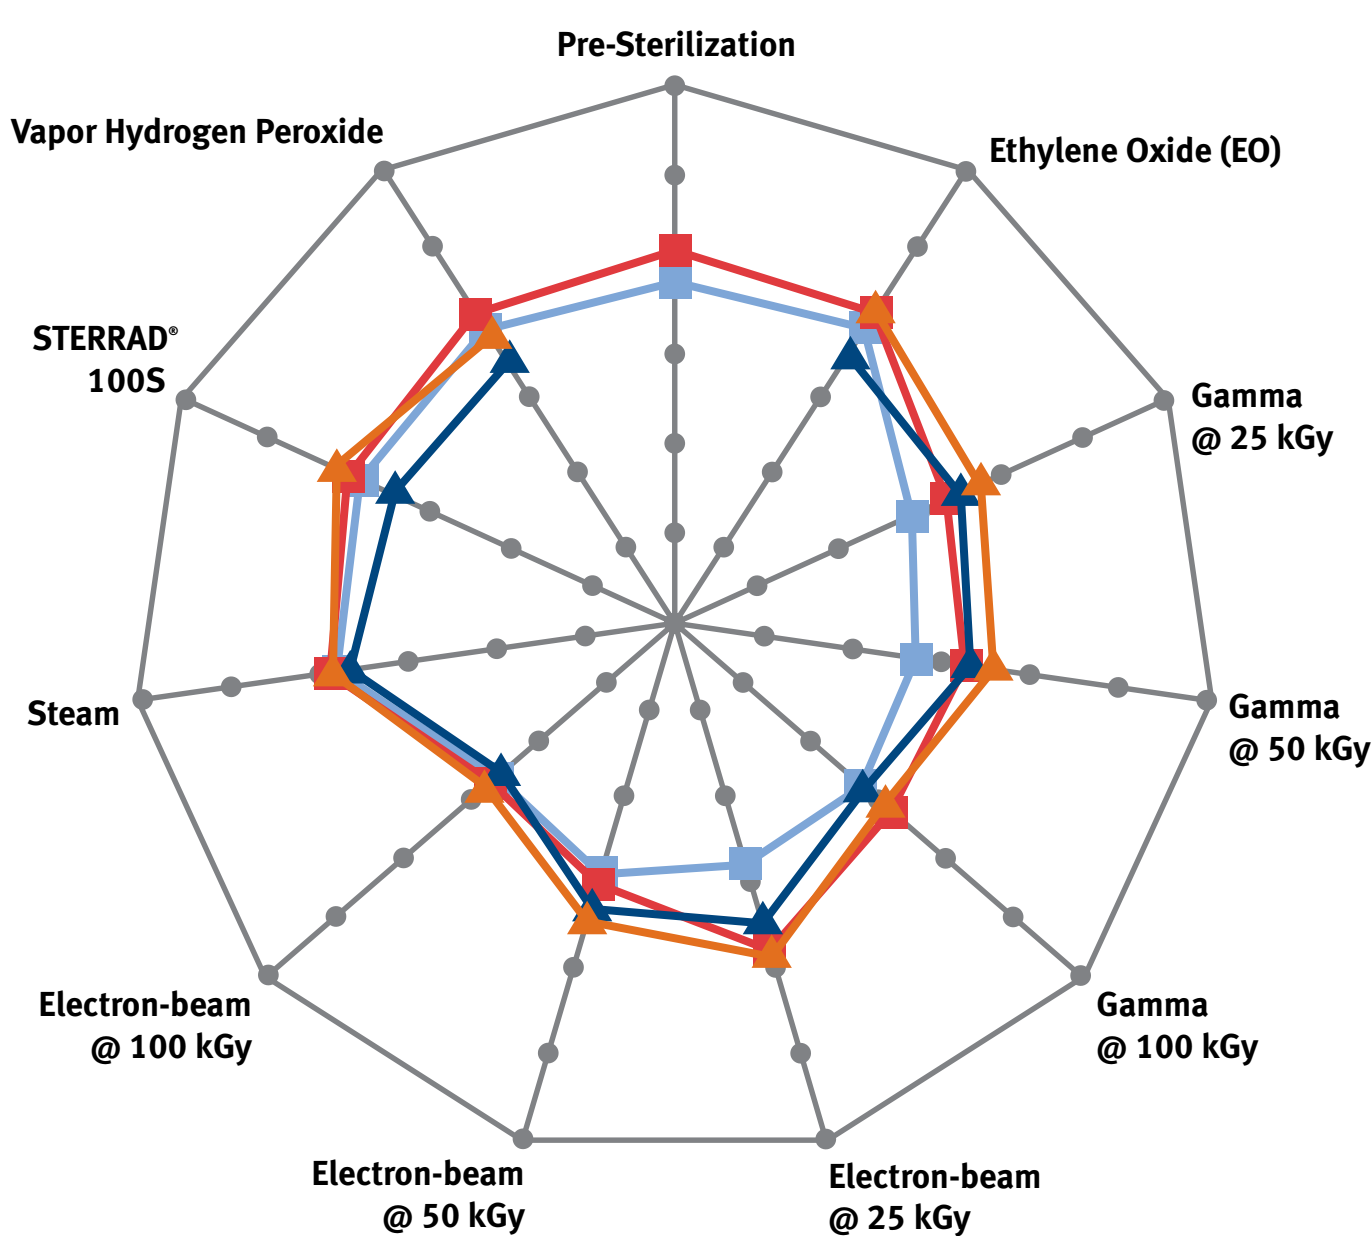


Tyvek.

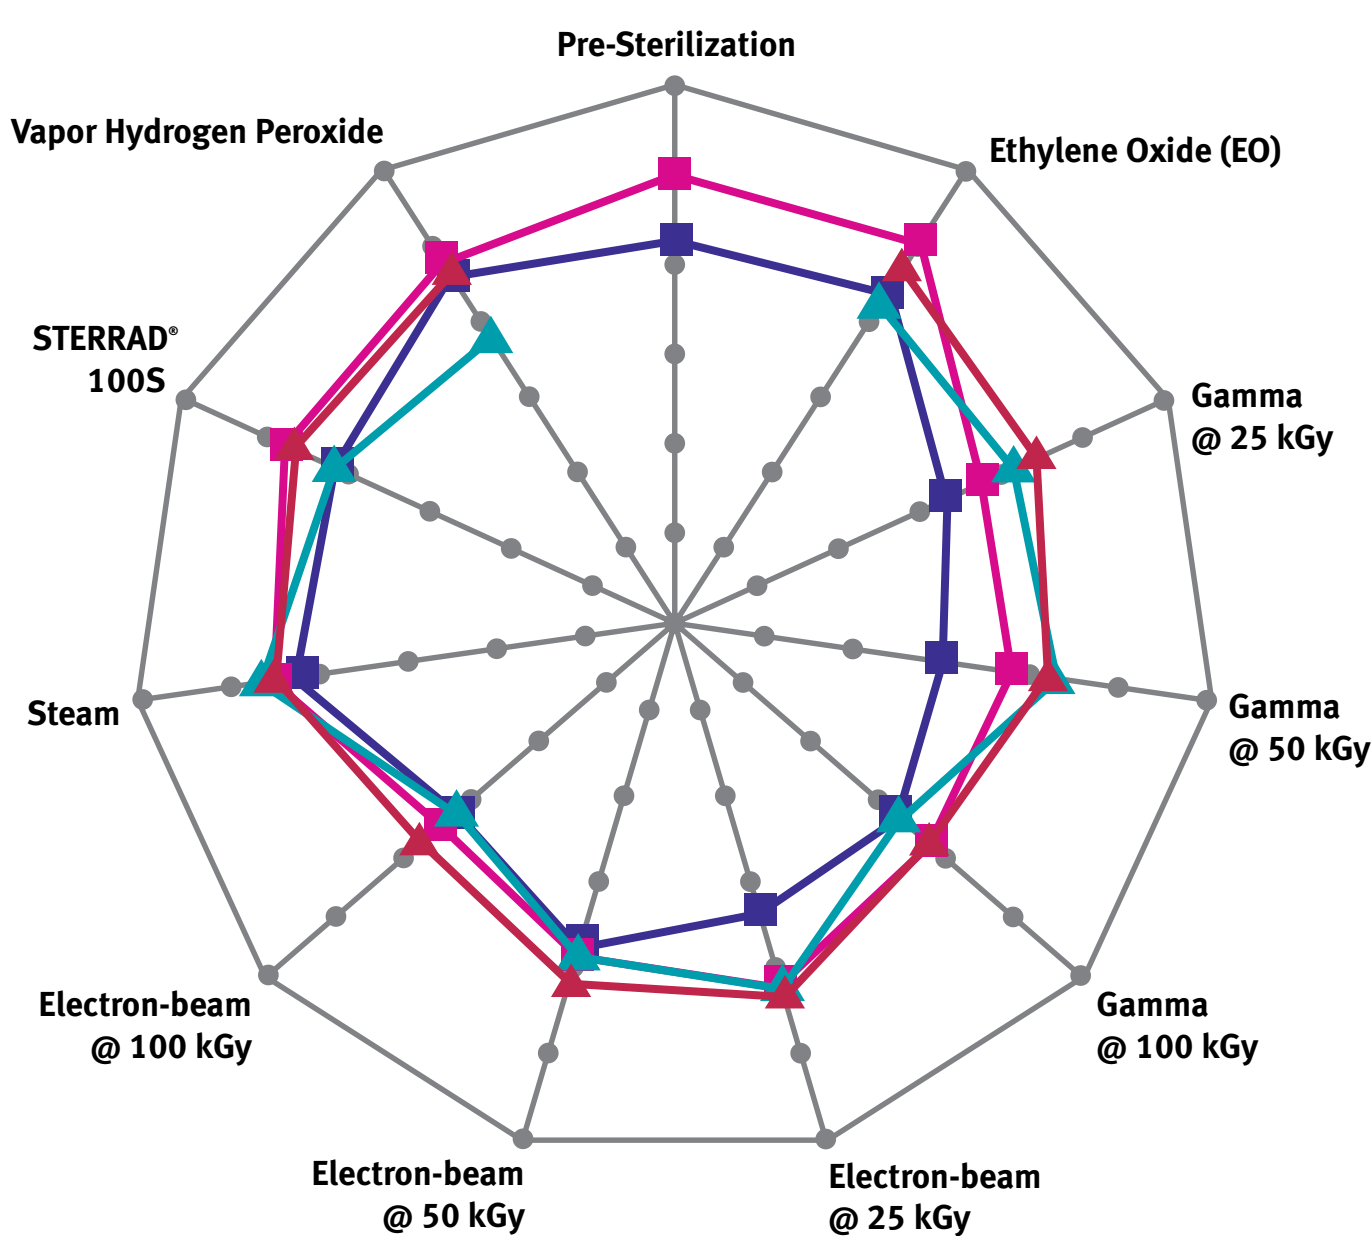

Transition Protocol material performance is equivalent to, or better than, current Tyvek®.

Effects of Sterilization and 1-Year Real-Time Aging on Material Elongation (MD) for 1073B

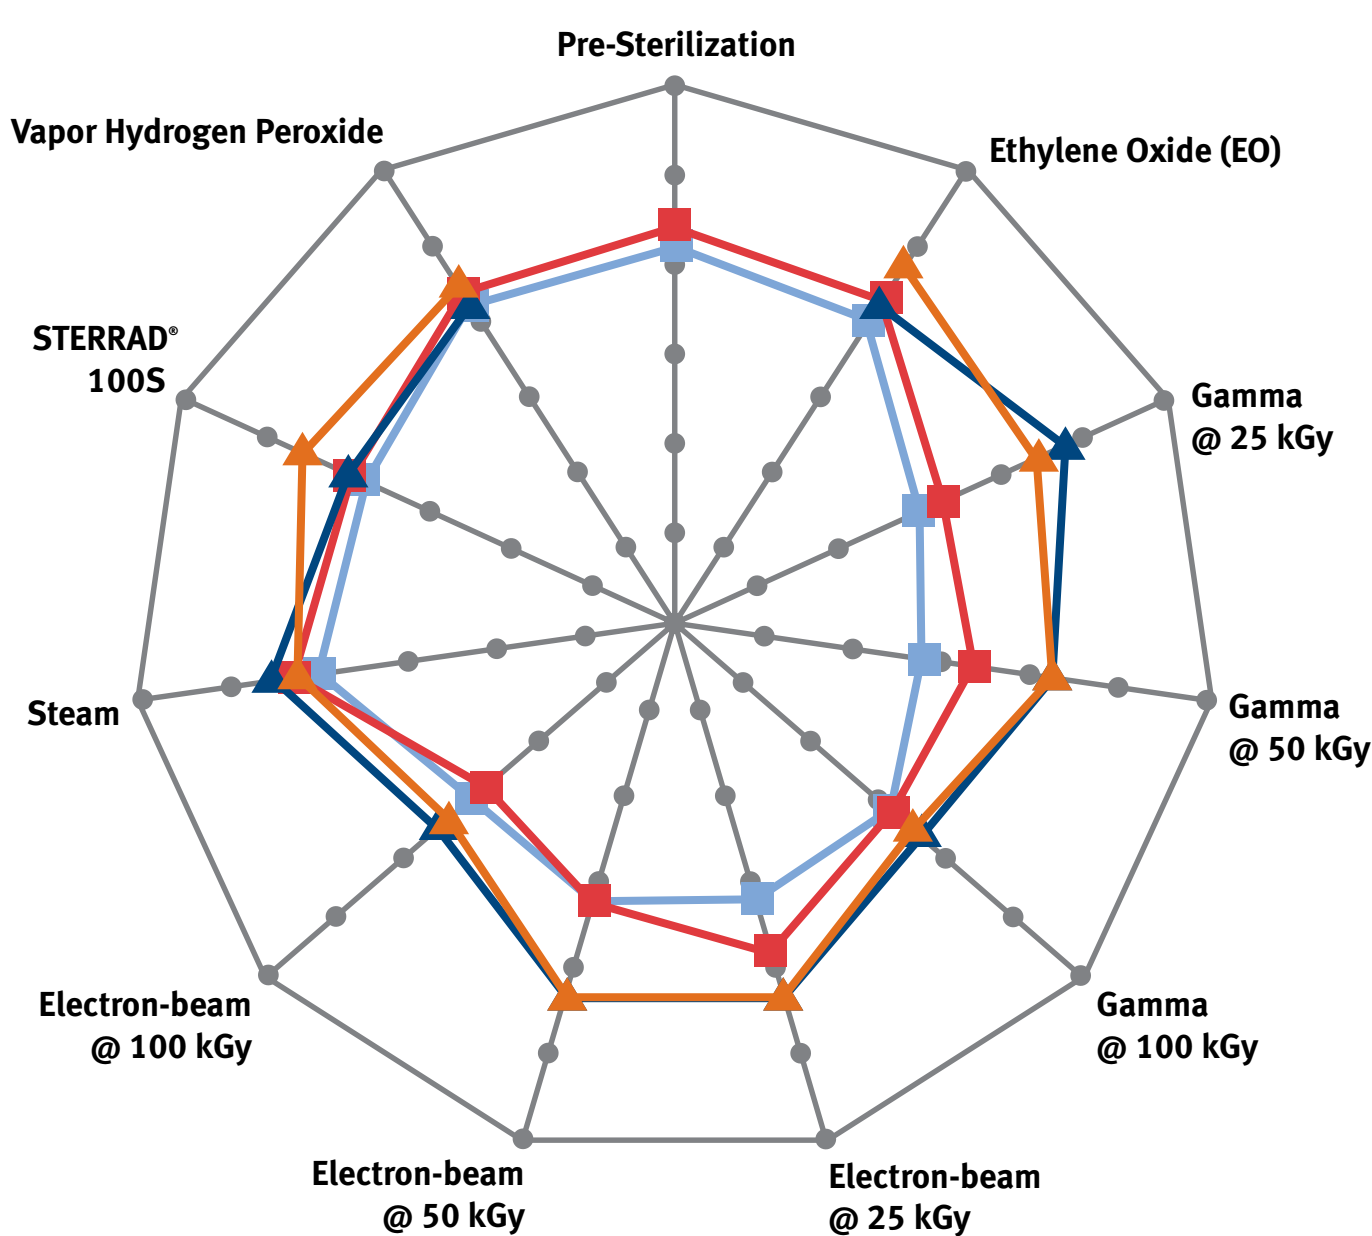


Transition Protocol material performance is equivalent to, or better than, current Tyvek®.

Effects of Sterilization and 1-Year Real-Time Aging on Material Elongation (CD) for 1073B



Tyvek.

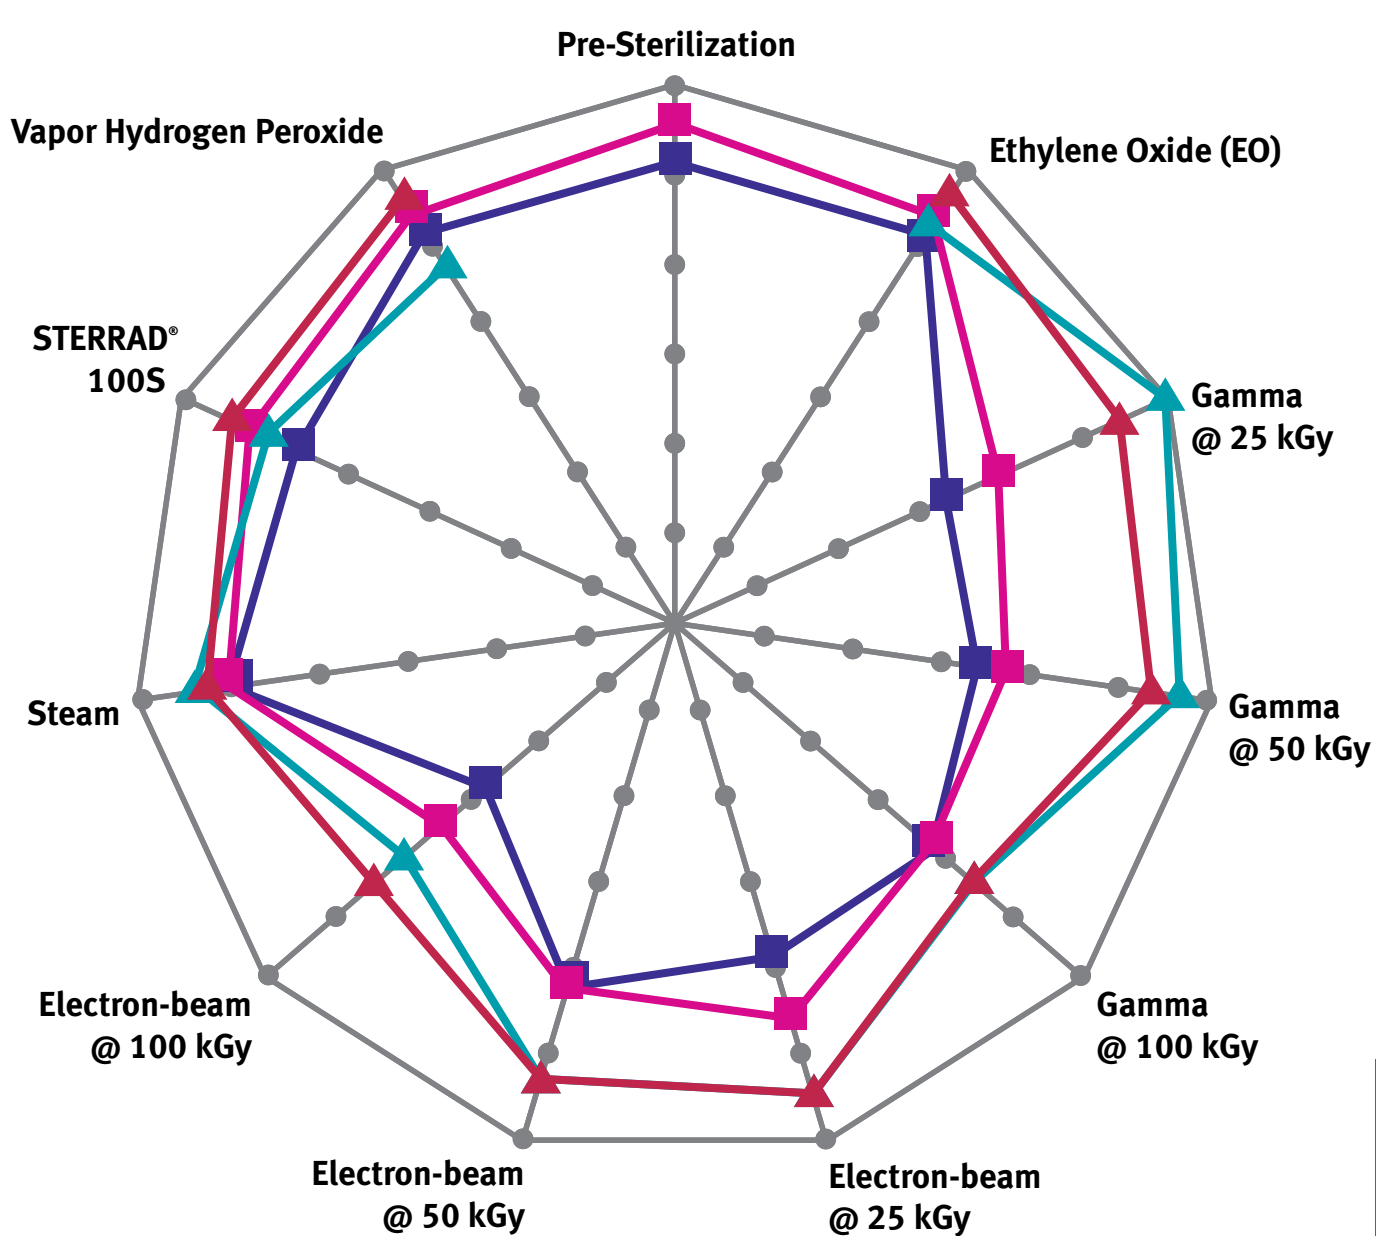


- ▲ Transition Protocol Material 1-Year Real-Time Aging
- ▲ Control 1-Year Real-Time Aging
- Transition Protocol Material 0-Year
- Control 0-Year

ASTM D5034
 Control = DuPont™ Tyvek® 1073B
 Center point = 0%
 Outer point = 30%
 CD = Cross Direction

Transition Protocol material performance is equivalent to, or better than, current Tyvek®.

Effects of Sterilization and 1-Year Real-Time Aging on Material Puncture Strength for 1073B

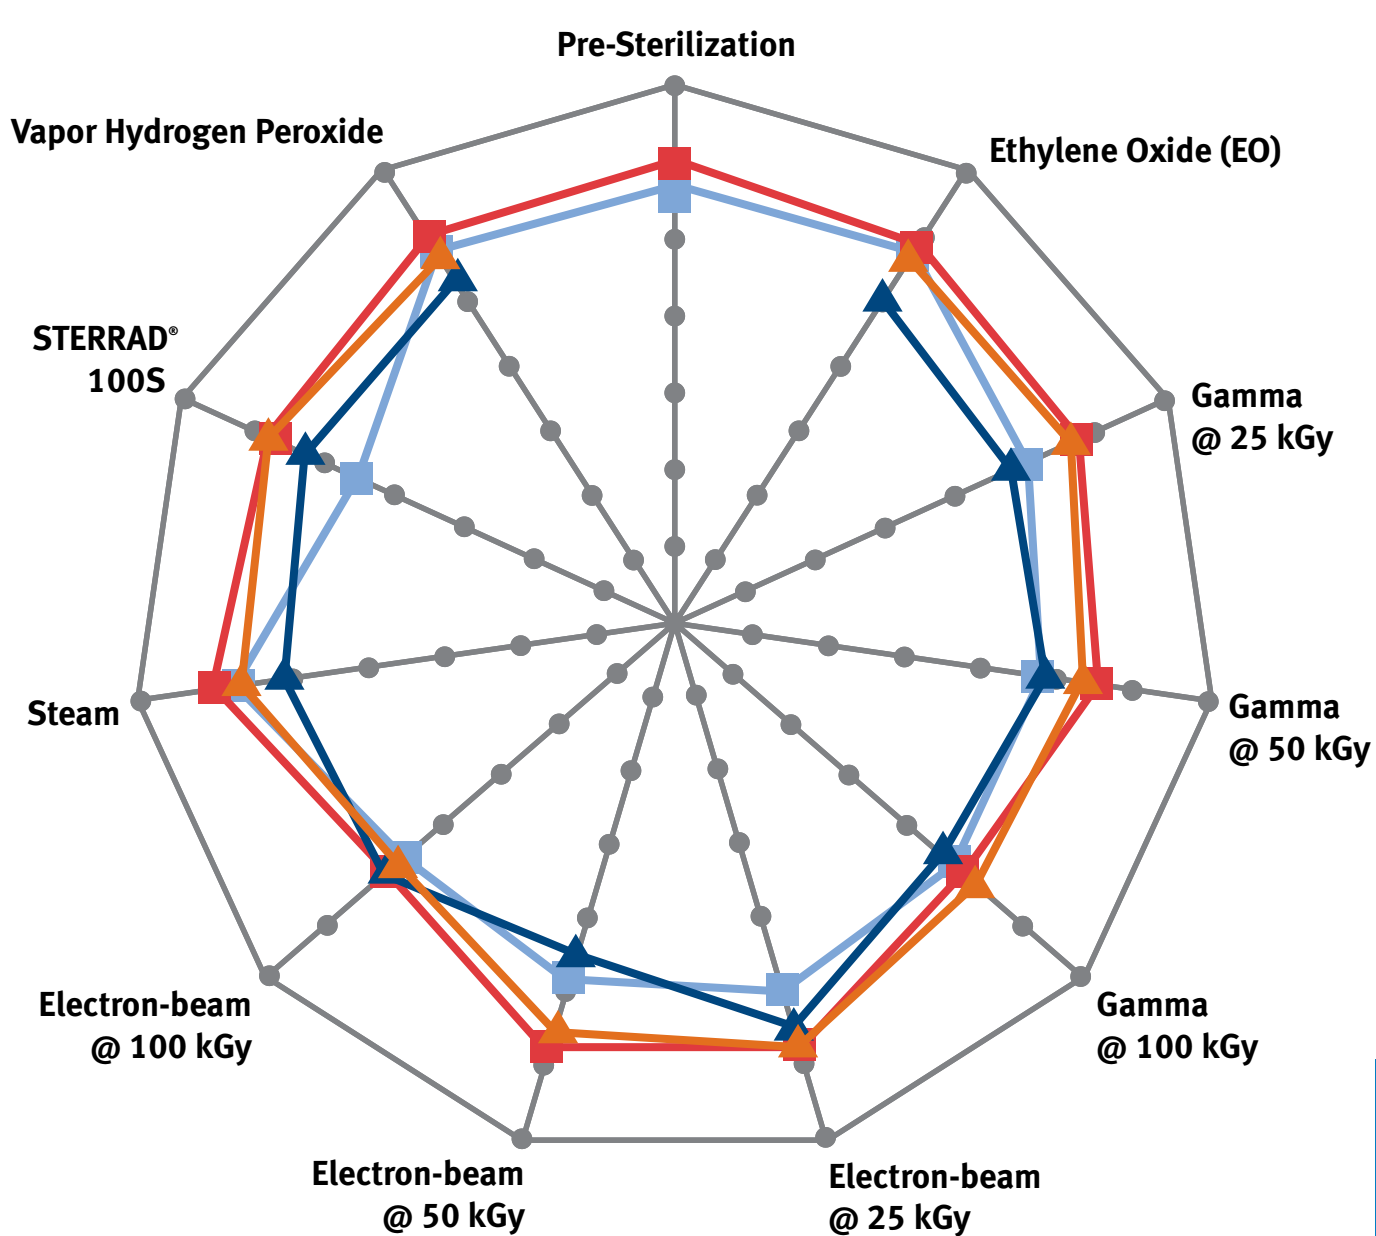

Transition Protocol material performance is equivalent to, or better than, current Tyvek®.